

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2304
CALIBRATION DATE: 25-Oct-07

SBE4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Seimens/meter

GHIJ COEFFICIENTS

g = -1.04623113e+001
h = 1.58182324e+000
i = -3.45795042e-003
j = 3.62906198e-004
CPcor = -9.5700e-008 (nominal)
CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 1.25916623e-007
b = 1.57237236e+000
c = -1.04425424e+001
d = -8.02503389e-005
m = 7.1
CPcor = -9.5700e-008 (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.57709	0.00000	0.00000
-1.0000	34.8025	2.80357	4.94618	2.80354	-0.00003
1.0000	34.8030	2.97494	5.05508	2.97496	0.00002
15.0000	34.8034	4.27020	5.81192	4.27023	0.00003
18.5000	34.8038	4.61689	5.99813	4.61686	-0.00003
29.0000	34.8000	5.69995	6.54549	5.69994	-0.00000
32.5000	34.7918	6.07220	6.72318	6.07221	0.00001


Conductivity = $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$ Siemens/meter

Conductivity = $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$ Siemens/meter

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correction

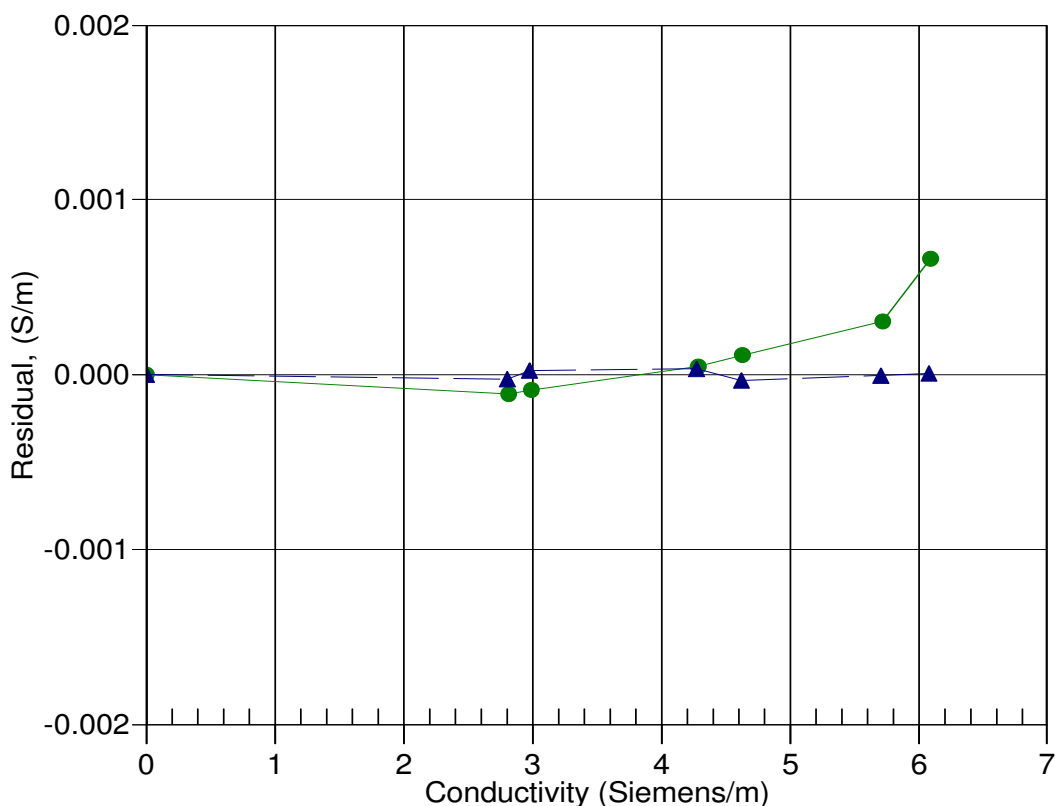

06-Oct-06 0.9999533
25-Oct-07 1.0000000