

# SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 3089  
CALIBRATION DATE: 26-Sep-08

SBE4 CONDUCTIVITY CALIBRATION DATA  
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

## GHIJ COEFFICIENTS

g = -1.03616620e+001  
h = 1.39306560e+000  
i = 2.99355157e-004  
j = 4.32981445e-005  
CPcor = -9.5700e-008 (nominal)  
CTcor = 3.2500e-006 (nominal)

## ABCDM COEFFICIENTS

a = 2.12929325e-004  
b = 1.39328223e+000  
c = -1.03619619e+001  
d = -8.48173542e-005  
m = 3.5  
CPcor = -9.5700e-008 (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.72616	0.00000	0.00000
-1.0001	34.8696	2.80846	5.24818	2.80843	-0.00003
1.0000	34.8693	2.98006	5.36391	2.98010	0.00003
14.9999	34.8708	4.27758	6.16848	4.27756	-0.00002
18.4999	34.8704	4.62476	6.36648	4.62477	0.00001
29.0000	34.8689	5.70996	6.94880	5.70996	-0.00000
32.5000	34.8645	6.08344	7.13815	6.08344	0.00000


Conductivity =  $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$  Siemens/meter

Conductivity =  $(af^m + bf^2 + c + dt) / [10 (1 + \epsilon p)]$  Siemens/meter

t = temperature[°C]; p = pressure[decibars];  $\delta$  = CTcor;  $\epsilon$  = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correction

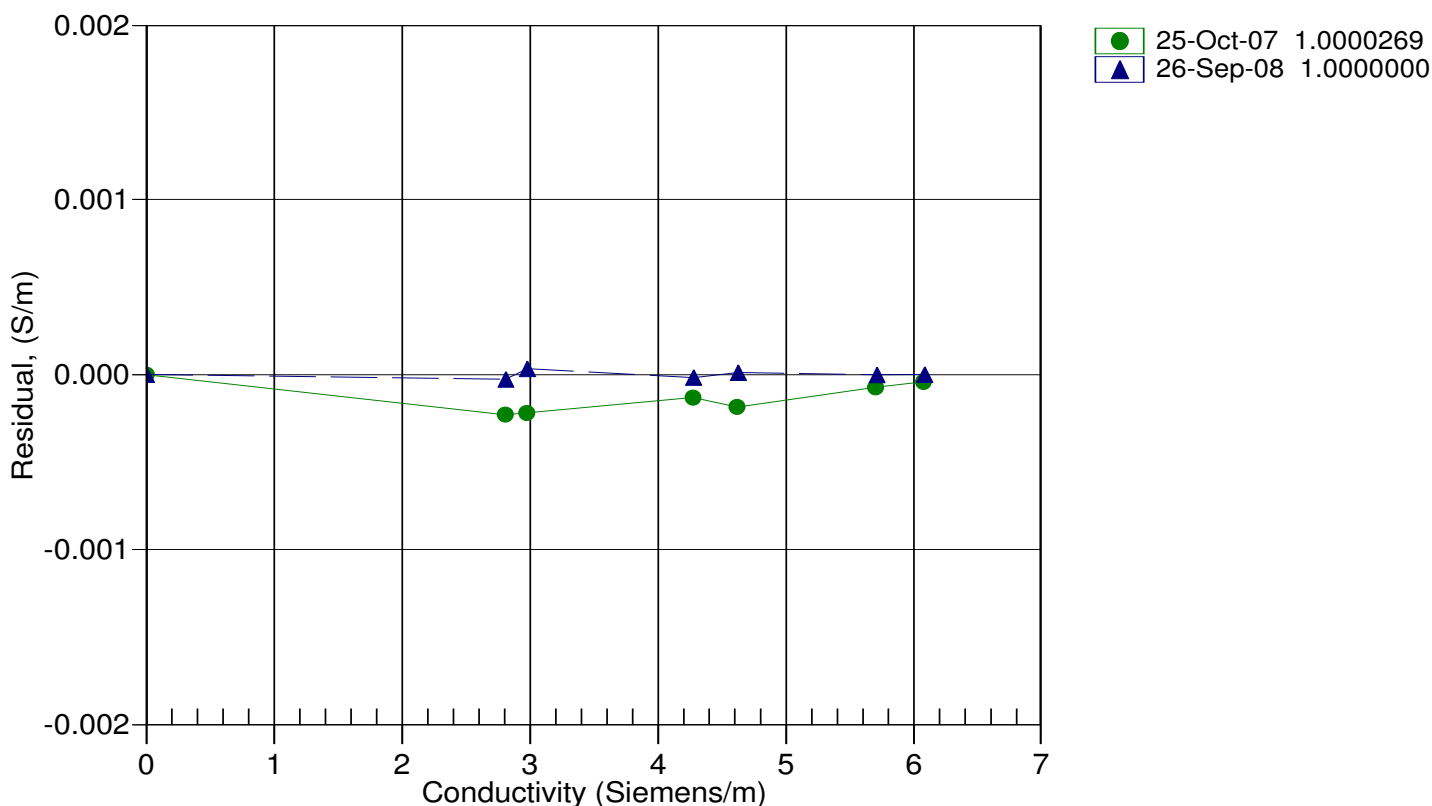



## SEA-BIRD ELECTRONICS, INC.

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

### Conductivity Calibration Report

Customer:	Woods Hole Oceanographic Institution		
Job Number:	51761	Date of Report:	9/26/2008
Model Number	SBE 04C	Serial Number:	043089

*Conductivity sensors are normally calibrated 'as received', without cleaning or adjustments, allowing a determination of sensor drift. If the calibration identifies a problem or indicates cell cleaning is necessary, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.*

*An 'as received' calibration certificate is provided, listing the coefficients used to convert sensor frequency to conductivity. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'slope' allows small corrections for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair or cleaning apply only to subsequent data.*

#### 'AS RECEIVED CALIBRATION'

☒ Performed ☐ Not Performed

Date: 9/26/2008

Drift since last cal:

+0.00010

PSU/month\*

Comments:

#### 'CALIBRATION AFTER CLEANING & REPLATINIZING'

☐ Performed ☒ Not Performed

Date:

Drift since Last cal:

PSU/month\*

Comments:

*\*Measured at 3.0 S/m*

*Cell cleaning and electrode replatinizing tend to 'reset' the conductivity sensor to its original condition. Lack of drift in post-cleaning-calibration indicates geometric stability of the cell and electrical stability of the sensor circuit.*